


Quick Guide QuantIFERON®-TB Gold Blood Collection

Incubate at Laboratory


For comprehensive instructions for use, please refer to the Package Insert, available in up to 25 different languages, on www.cellestis.com.

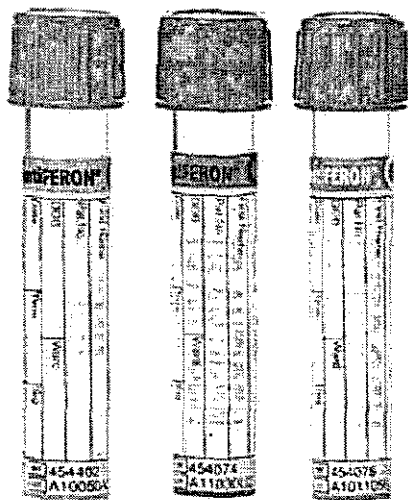

Grey Cap Red Cap Lav Cap

①

BLOOD COLLECTION

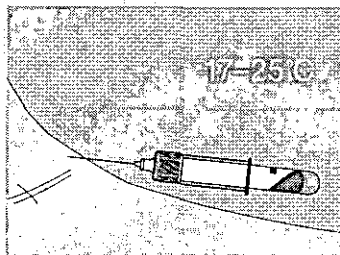

Collect 1mL blood by venipuncture into each QFT blood collection tube.

Tubes should be at 17–25°C at the time of blood filling.

Tubes fill slowly—hold tube on needle for 2–3 seconds after flow ceases.

If blood level is not close to the black mark on the side of the tube label, obtain another sample.


Technical Tip

Butterfly needles—prime tubing with a “purge” tube (not supplied) before filling QFT tubes.



②

BLOOD COLLECTION

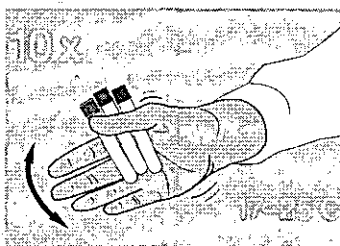

Immediately after filling, shake tubes ten (10) times just firmly enough to ensure that the inner surface of the tube is coated in blood (to solubilize antigens on tube walls).


Over-energetic shaking may cause gel disruption and could lead to aberrant results.

Label tubes appropriately.



③

SHIPPING / INCUBATION

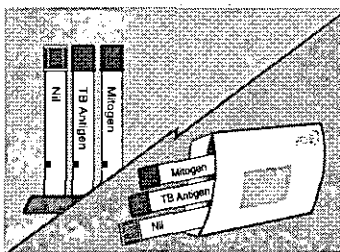

Incubate at Laboratory

Ship tubes to laboratory at 17–27°C.

Blood must be incubated at 37°C as soon as possible (and within 16 hours of collection).

For more information on QFT in your area, please visit www.cellestis.com.
World Headquarters | Cellestis Limited | Email: info@cellestis.com | Tel: +61 3 8527 3500

⚠ WARNING: Standard blood handling precautions apply.